

PolyLink Protein Coupling Kit

for COOH Microspheres

DESCRIPTION

Carboxyl (COOH) microspheres can be used for covalent coupling of proteins by activating the carboxyl groups with water-soluble carbodiimide. The carbodiimide reacts with the carboxyl group to create an active ester that is reactive toward primary amines on the protein of interest.

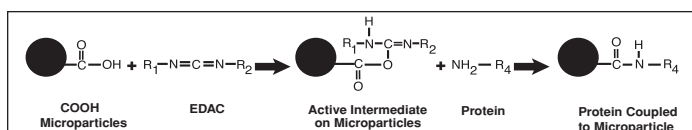


Figure 1

Polysciences, Inc. offers the PolyLink Protein Coupling Kit for COOH Microspheres for the covalent coupling of proteins to carboxylated microspheres. The procedure that follows has been optimized for polymer microspheres 1µm or larger. The contents of the kit are sufficient for 50 coupling reactions using 200-500µg of protein per reaction. The kit has been optimized using purified IgG as the coupling protein.

MATERIAL

Material Supplied

- PolyLink Coupling Buffer (50mM MES, pH 5.2; 0.05% Proclin® 300): 55ml
- PolyLink Wash/Storage Buffer (10mM Tris, pH 8.0; 0.05% Bovine Serum Albumin; 0.05% Proclin 300): 45ml
- PolyLink EDAC (Carbodiimide): 750mg. *Note:* Store powder desiccated at -20°C. Flood headspace with N₂ gas for best preservation. Warm the sealed vial to room temperature in a desiccator to avoid condensate formation in the bottle. Make working solutions just before use.

Material Required

- Carboxylated polystyrene or silica microspheres
- Centrifuge
- Test tubes

PROCEDURE

Researchers are advised to optimize the protein to microsphere ratio and incubation times for their particular protein.

1. Warm microspheres, PolyLink Coupling Buffer and PolyLink Wash/Storage Buffer to room temperature.
2. Pipet 12.5mg of microspheres into a 1.5-2ml polypropylene microcentrifuge tube.
3. Pellet the microspheres via centrifugation for 5-10 minutes at

approximately 500-1000 x G. *Note:* Centrifugation times will vary according to the size of the particle.

4. Resuspend microsphere pellet in 0.4ml of PolyLink Coupling Buffer.
5. Pellet again via centrifugation for 5-10 minutes at approximately 500-1000 x G.
6. Resuspend the microsphere pellet in 0.17ml of PolyLink Coupling Buffer.
7. Just before use, prepare a 200 mg/ml EDAC solution by dissolving 10mg PolyLink EDAC in 50µl PolyLink Coupling Buffer. Use immediately.
8. Add 20µl of the EDAC solution to the microsphere suspension.
9. Mix gently end-over-end or briefly vortex. Allow the activation step to proceed for 15 minutes.
10. Add protein equivalent to 200-500µg. This may be prepared as 1 - 5mg/ml protein in coupling buffer. Mix gently end-over-end or briefly vortex. *Note:* The amount of protein bound to the microspheres is dependent on the concentration of protein in solution and on the size of the microspheres. For an example of this relationship, please refer to Figure 2.
11. Incubate for 30-60 minutes at room temperature with gentle mixing. *Note:* End-over-end mixing is best. Longer incubation times may result in greater protein binding. See Figure 3.
12. Centrifuge mixture for 10 minutes at approximately 500-1000 x G. Save this supernatant for determination of the amount of bound protein.
13. Resuspend microsphere pellet in 0.4ml PolyLink Wash/Storage Buffer.
14. Repeat Steps 12-13, combining supernatants for use in bound protein calculation.
15. Store particles at 4°C in PolyLink Wash/Storage Buffer.

NOTES

Magnetic Particles

Carboxy-modified superparamagnetic particles are also compatible with the PolyLink kit and magnetic separation may be substituted for centrifugation steps in the procedure when magnetic particles are used.

Use of PolyLink with Other Microspheres

The PolyLink kit may be used with carboxylated silica or polymer/magnetic (e.g. ProMag™) microspheres. In those instances, magnetic separation may be used for superparamagnetic microspheres, or centrifugation steps may be modified for silica, taking their greater density into consideration.

Calculation of the Amount of Bound Protein

The amount of protein added in Step 10 less the amount of protein left

in the supernatants in Steps 12 and 14 represents the amount of protein bound to the microparticles. Protein concentrations of the starting solution and supernatants after binding may be determined by measuring the absorbance at 280nm or by utilizing commercial protein assay kits. *Note:* If measuring absorbance at 280nm, solutions used for calculation of bound protein should not contain EDAC. EDAC may contribute to the absorbance at 280nm.

Example:

$$\left[\begin{array}{l} \mu\text{g of protein} \\ \text{in starting} \\ \text{solution} \end{array} \right] - \left[\begin{array}{l} \mu\text{g of protein in} \\ \text{wash supernatants} \end{array} \right] \Bigg/ \text{mg of} \\ \text{microparticles}$$

===== $\mu\text{g of protein bound/mg microparticles}$

$$\left[\begin{array}{l} 100\mu\text{g of} \\ \text{protein in} \\ \text{starting solution} \end{array} \right] - \left[\begin{array}{l} 45\mu\text{g of protein in} \\ \text{wash supernatants} \end{array} \right] \Bigg/ 12.5\text{mg of} \\ \text{microparticles}$$

===== 4.4 $\mu\text{g of protein bound/mg microparticles}$

TRADEMARKS AND REGISTERED TRADEMARKS

1. ProClin® is a registered trademark of Rohm & Haas Company.
2. ProMag™ is a trademark of Polysciences, Inc.

STORAGE

Store PolyLink buffers at 2-8°C. Coated particles should be stored at 2-8°C in PolyLink Wash/Storage Buffer or other suitable storage buffer. Store EDAC desiccated at -20°C. Freezing of particles may result in irreversible aggregation and loss of binding activity.

These products are for research use only and are not intended for use in humans or for *in vitro* diagnostic use.

Expected Results

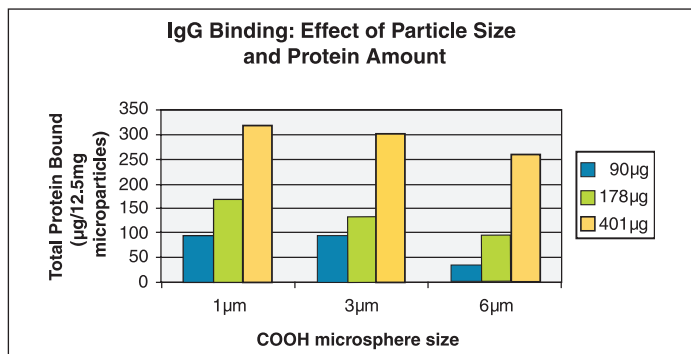


Figure 2: The Effect of Particle Size on Protein Binding at Equal Solids. Three different sizes of carboxyl microspheres were exposed to three different levels of Goat anti-Rat IgG protein. The smaller particles represent more surface area per unit of mass and therefore bind more total protein.

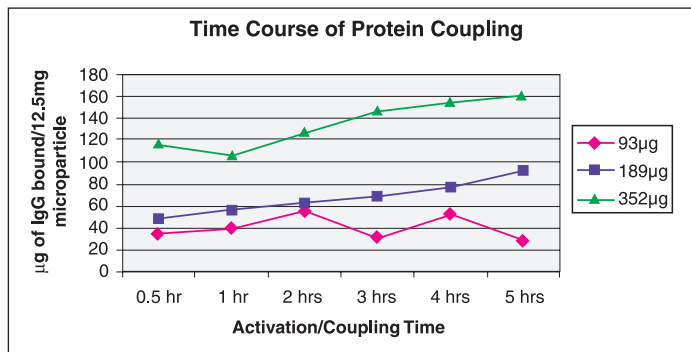


Figure 3: Time Course of Protein Binding. Three different levels of protein were used in the PolyLink procedure using 3µm carboxyl microspheres. As expected, more input protein results in more protein bound. The majority of the protein binding occurs in the first 30 minutes.

ORDERING INFORMATION

Cat. #	Description	Size
24350-1	PolyLink Protein Coupling Kit	1 kit

TO ORDER

In The U.S. Call: 1(800) 523-2575 • (215) 343-6484
 In The U.S. Fax: 1(800) 343-3291 • (215) 343-0214
 In Germany Call: +(49) 6221-765767
 In Germany Fax: +(49) 6221-764620
 In Asia Call: (886) 2 8712 0600
 In Asia Fax: (886) 2 8712 2677

Order online anytime at www.polysciences.com

Should any of our materials fail to perform to our specifications, we will be pleased to provide replacements or return the purchase price. We solicit your inquiries concerning all needs for life sciences work. The information given in this bulletin is to the best of our knowledge accurate, but no warranty is expressed or implied. It is the user's responsibility to determine the suitability for their own use of the products described herein, and since conditions of use are beyond our control, we disclaim all liability with respect to the use of any material supplied by us. Nothing contained herein shall be construed as a recommendation to use any product or to practice any process in violation of any law or any government regulation.